

Sign in to the Align Global Gallery Dashboard to submit an IPE treatment for review.

At this time, only IPE cases are being accepted into the Gallery. More treatment options will be available soon.

align
Align Global Gallery

Sign In

Email Address

Password

Forget password ?

Sign In

New doctor account creation is coming soon.

Reset your password to begin

The email address should be the same that you used on the previous Align Global Gallery



The screenshot shows the Align dashboard interface. On the left is a dark blue sidebar with the 'align' logo at the top. Below the logo, the word 'MAIN' is displayed, followed by a 'Dashboard' button with a home icon. The main content area has a light blue header with a hamburger menu icon on the left, the text 'Welcome back, Christian Ross', and a green 'Edit your profile' link with an arrow pointing to a user profile dropdown menu. The dropdown menu includes a notification bell icon, a profile icon, the name 'Christian Ross', the role 'Super Admin', and two options: 'Profile' and 'Log Out'. Below the header is a section titled 'Approved & Published Treatments' which is currently empty. A green callout box with an arrow points to the 'Dashboard' button in the sidebar, containing the text: 'You can always click here to return to your Dashboard.' At the bottom of the main content area, there is a large green heading 'Your Dashboard' followed by the text 'More information will show here as you have more submissions to the Gallery'. The footer contains the copyright notice '© Align Technology 2024. All rights reserved.'

Your Dashboard

Your Edit Profile Screen

You should be able to access this screen at any time by clicking on your name in the top-right corner and selecting Profile.

Take a moment to verify or add any missing information before moving on. Don't forget to hit the Save button on the bottom-right.

align MAIN Dashboard Christian Ross Super Admin

Christian Ross

Verify or update your information

Add a profile image

Profile Created: System 6/29/21

Personal Information

Prefix: Dr. First Name: Last Name: Email address: Role: Submitting Doctor Market: USA Timezone: (GMT-06:00) Central Time (US & Canada) ClinID: Website: Type of doctor: Orthodontist General practitioner Change Password: New Password: Confirm Password:

Office information

Name: Contact person: Address: 1 City: New York State: NY Zip code: 10019 Phone number: I am the contact person for this clinic

University Information

Name: Address: City: State: Zip code: Website: Faculty advisor: Year of graduation:

Save Profile

© Align Technology 2024. All rights reserved.

Dashboard

As you submit Treatments to the Align Global Gallery, more information will appear on your Dashboard.

Click the Add New Treatment button to begin a submission.

The screenshot shows the Align dashboard interface. On the left is a dark blue sidebar with the 'align' logo at the top. Below the logo, the word 'MAIN' is displayed, followed by a 'Dashboard' button with a home icon. The main content area has a light blue header with a hamburger menu icon on the left, a welcome message 'Welcome back, Christian Ross', a green link 'Click here to begin a new IPE submission to the Gallery', and a purple 'Add New Treatment' button. Below the header is a white box titled 'Approved & Published Treatments' which is currently empty. At the bottom right of the main area, there is a copyright notice: '© Align Technology 2024. All rights reserved.' In the top right corner of the dashboard, there is a notification bell icon with a '0' and a user profile for 'Christian Ross Super Admin'.

Treatment Submission

To begin an IPE treatment submission, click on either button to start the process.

The screenshot displays the Align software interface for starting a treatment submission. The sidebar on the left contains the 'align' logo and navigation options: 'MAIN', 'Dashboard', 'Patient Information', 'Legal Documents', 'Treatment Information', and 'Status'. The main content area is titled 'Patient Treatment' and 'Begin Treatment Submission'. Under the 'Treatment Information' section, there is a heading 'Add a treatment' and the instruction 'Choose one of the available treatments below.' Two buttons are highlighted with green boxes: one labeled 'IPE' with 'Invisalign Palatal Expander' below it, and another labeled 'Add Treatment Option' with a dropdown arrow and 'Invisalign Palatal Expander' below it. A green arrow labeled 'Either option' points to both buttons. The footer contains the copyright notice '© Align Technology 2024. All rights reserved.'

Patient Information

Enter all required Patient Information for this treatment.

Click the Save button before proceeding.

The screenshot shows the Align software interface. On the left is a dark blue sidebar with the 'align' logo and a 'MAIN' menu containing 'Dashboard'. A green arrow points to '3. Move to Legal Documents' in the sidebar. The main content area is titled 'Patient Treatment' and 'Submission Process: Patient Info'. It features a 'Patient Information' section with a profile card for 'Christian Ross, NA | USA' and a 'View' link. Below this is a form with fields for 'Age Group', 'Invisalign Patient ID Number (PID)', 'Gender' (Male/Female), 'Patient Birth Date', and 'Initials'. A green box highlights these form fields with the instruction '1. Complete the Patient Information for this submission'. Below the form is a 'Patient Profile Image' placeholder showing a set of teeth. A green arrow points to '2. Click Save' next to a purple 'Save' button in the bottom right corner.

Legal Documents

Upload PDF versions of Patient and Doctor Consent Releases from your computer.

Click the Save button before proceeding.

The screenshot shows the 'align' software interface. The top left has the 'align' logo. The top right shows a user profile for 'Christian Ross Super Admin'. The main header is 'Patient Treatment' with a sub-header 'Submission Process: Patient Consent'. A sidebar on the left contains navigation links: 'Patient Information', 'Legal Documents', 'Treatment Information', and 'Status'. A green arrow points to 'Treatment Information' with the text '3. Move to Treatment Info'. The main content area is titled 'Legal Documents' and contains a section '1. Upload required legal consent forms'. This section includes two document upload areas: 'Patient Consent and Release' and 'Doctor Consent and Release'. Each area has a 'Browse...' button and a 'No file selected.' message. To the right of each area is a 'DOWNLOAD' button with a PDF icon. A green box highlights the 'Patient Consent and Release' area. At the bottom right, a 'Save' button is highlighted with a green box and labeled '2. Click Save'. The footer contains the copyright notice: '© Align Technology 2024. All rights reserved.'

Treatment Information

Add all required and any additional information regarding this treatment. Upload images, select indications, modalities, expanders, etc.

Click the Save button before proceeding.

The screenshot shows the 'Submission Process: Treatment Info' form in the align software. The form is titled 'Treatment Information' and includes a sidebar with navigation options: Patient Information, Legal Documents, Treatment Information (selected), and Status. The main content area is for 'Invisalign Palatal Expander' and contains the following sections:

- Upload IPE Treatment Information for this Patient** (green header)
- Invisalign Palatal Expander** (title)
- Start Date** and **End Date** (input fields)
- Patient age** (input field) and **Length of treatment** (input field) at start of treatment in months
- Initial Scan code or ID** and **Final Scan code or ID** (input fields)
- Patient Chief Concern** (text area)
- Where any other treatment options used?** (text area)
- Clinical conditions** (dropdown menu) and **Clinical Conditions Comments** (text area)
- Treatment modalities used** (dropdown menu) and **Treatment Modalities Comments** (text area)
- Palatal Expanders** (dropdown menu) with a table for expansion details:

	Number of Expanders	Planned Expansion (mm)	Expansion Protocol (duration in days)	Expander Change Frequency
Initial	0	0	0	0
Additional	0	0		
- Palatal Holders** (dropdown menu) with a table for holder details:

	Number of Holders	Holder Protocol (duration in weeks)	Holder Change Frequency
	0	0	0
- Initial Images** (dropdown menu) with tabs for Progress Images, Final Images, Post Images, Radiographs, and CBCT Images.
- Image Grid:**
 - Profile, Repose, Smile (patient photos)
 - Upper, Lower (dental arches)
 - Right, Anterior, Left (dental views)
 - External View, CBCT (radiographs)
- Treatment Submission Process** (dropdown menu) and **Treatment Submission Process Comments** (text area)
- Results Achieved** (text area)
- Additional Notes** (text area) with a note: "These notes will not be publicly viewable."
- Save** button (purple)

At the bottom right, there is a green callout: "2. Click Save" pointing to the Save button. The footer contains the copyright notice: "© Align Technology 2024. All rights reserved."

Option Selections

Several times you will see pop-up windows allowing you to choose detailed information about the treatment.

Click the Save button before proceeding.

The screenshot displays the Invisalign iTero software interface. A dark blue sidebar on the left contains the 'align' logo and a 'MAIN' menu with a 'Dashboard' option. A white pop-up window titled 'Select Clinical Indications' is centered on the screen, featuring a close button (X) in the top right corner. Inside the pop-up, there are five checkboxes: 'Asymmetric arches', 'Crossbite', 'Crowding', 'Narrow arches', and 'Smile width (narrow arches)'. Below these checkboxes, the text 'Submission Process: Treatment Selections' is displayed in green. To the right of this text are three buttons: 'Check All' (blue), 'Close' (grey), and 'Save' (purple). The background of the software interface is dimmed and shows various treatment planning options, including 'Treatment modalities used' with a 'Select' button, 'Treatment Modalities Comments' with a text area, 'Palatal Expanders' with a table of input fields, and 'Palatal Holders' with input fields. At the bottom of the interface, there are buttons for 'Initial Images', 'Progress Images', 'Final Images', 'Post Images', 'Radiographs', and 'CBCT Images', along with a 'Save' button in the bottom right corner.


	Number of Expanders	Planned Expansion (mm)	Expansion Protocol (duration in days)	Expander Change Frequency
Initial	0	0	0	0
Additional	0	0		

	Number of Holders	Holder Protocol (duration in weeks)	Holder Change Frequency
	0	0	0

Image Upload

As you select images to upload from your computer, you will be given the ability to crop and resize your photos.

Click the Save button before proceeding.

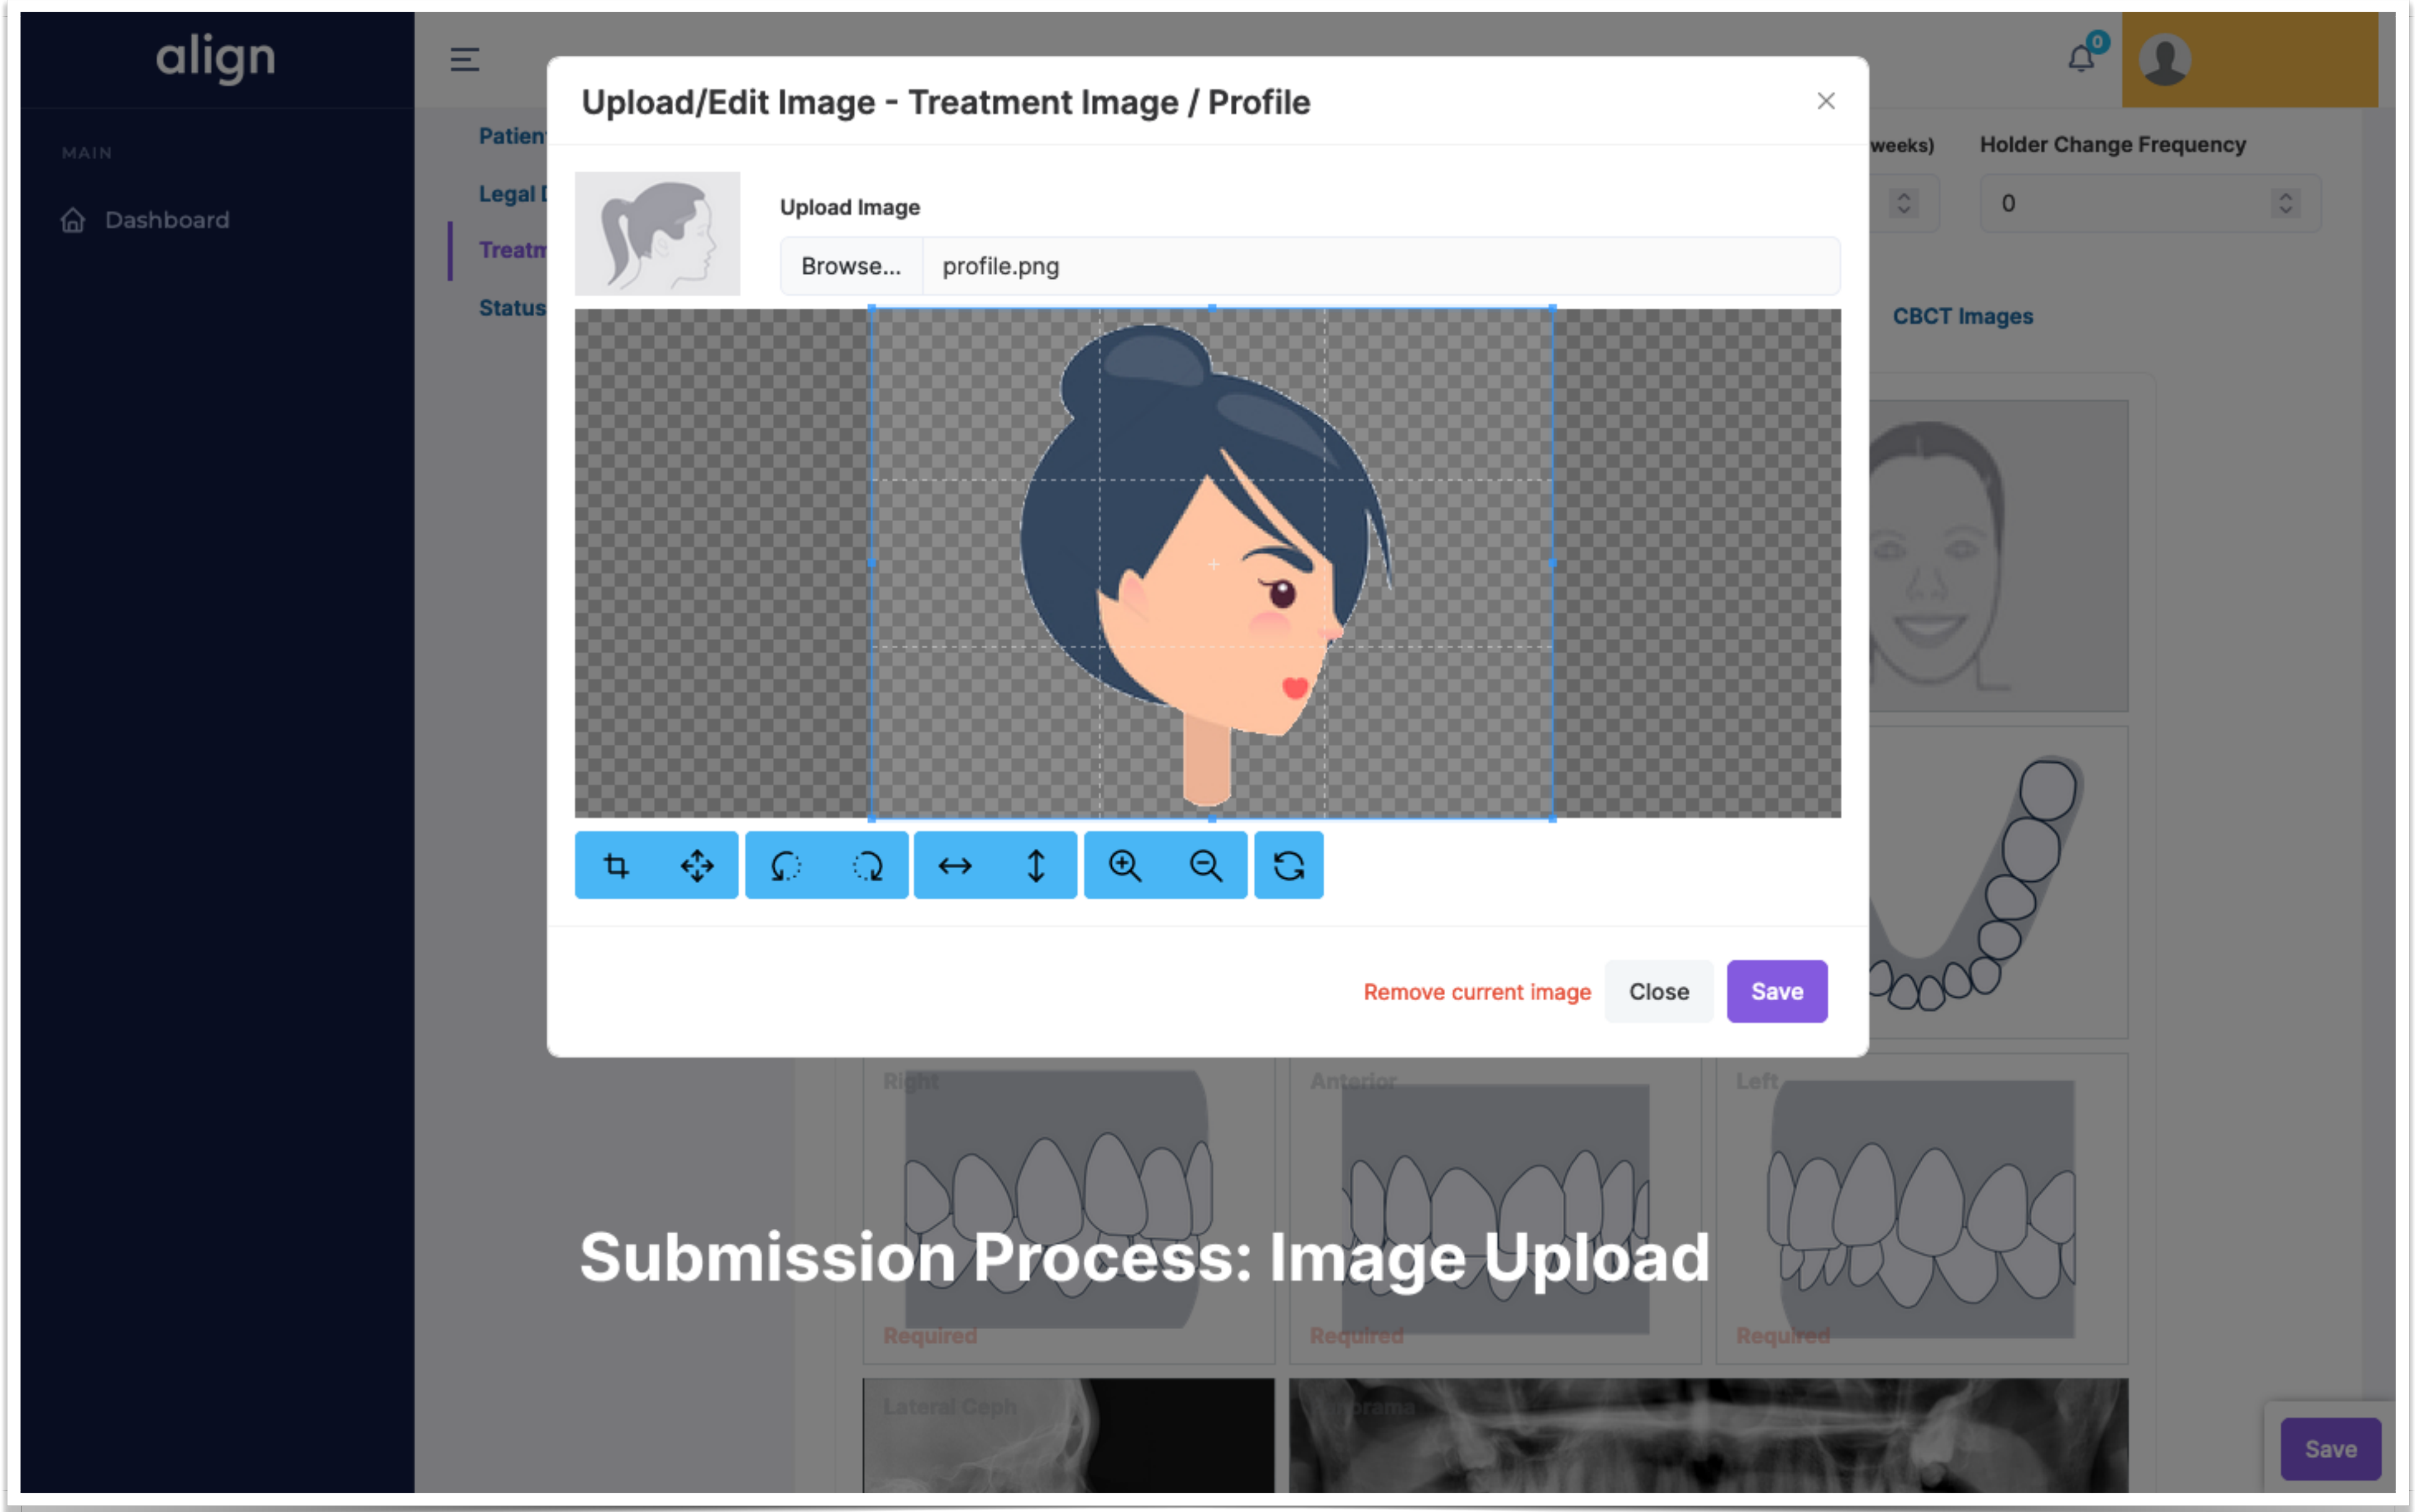


Submission Process: Image Upload

Required Information

As you go through the process of selecting and entering all of the treatment information, we give you a handy check-list of complete and incomplete fields that are required for submission. You will be unable to submit this treatment for review until all checkmarks are green.

Click the Save button before proceeding.

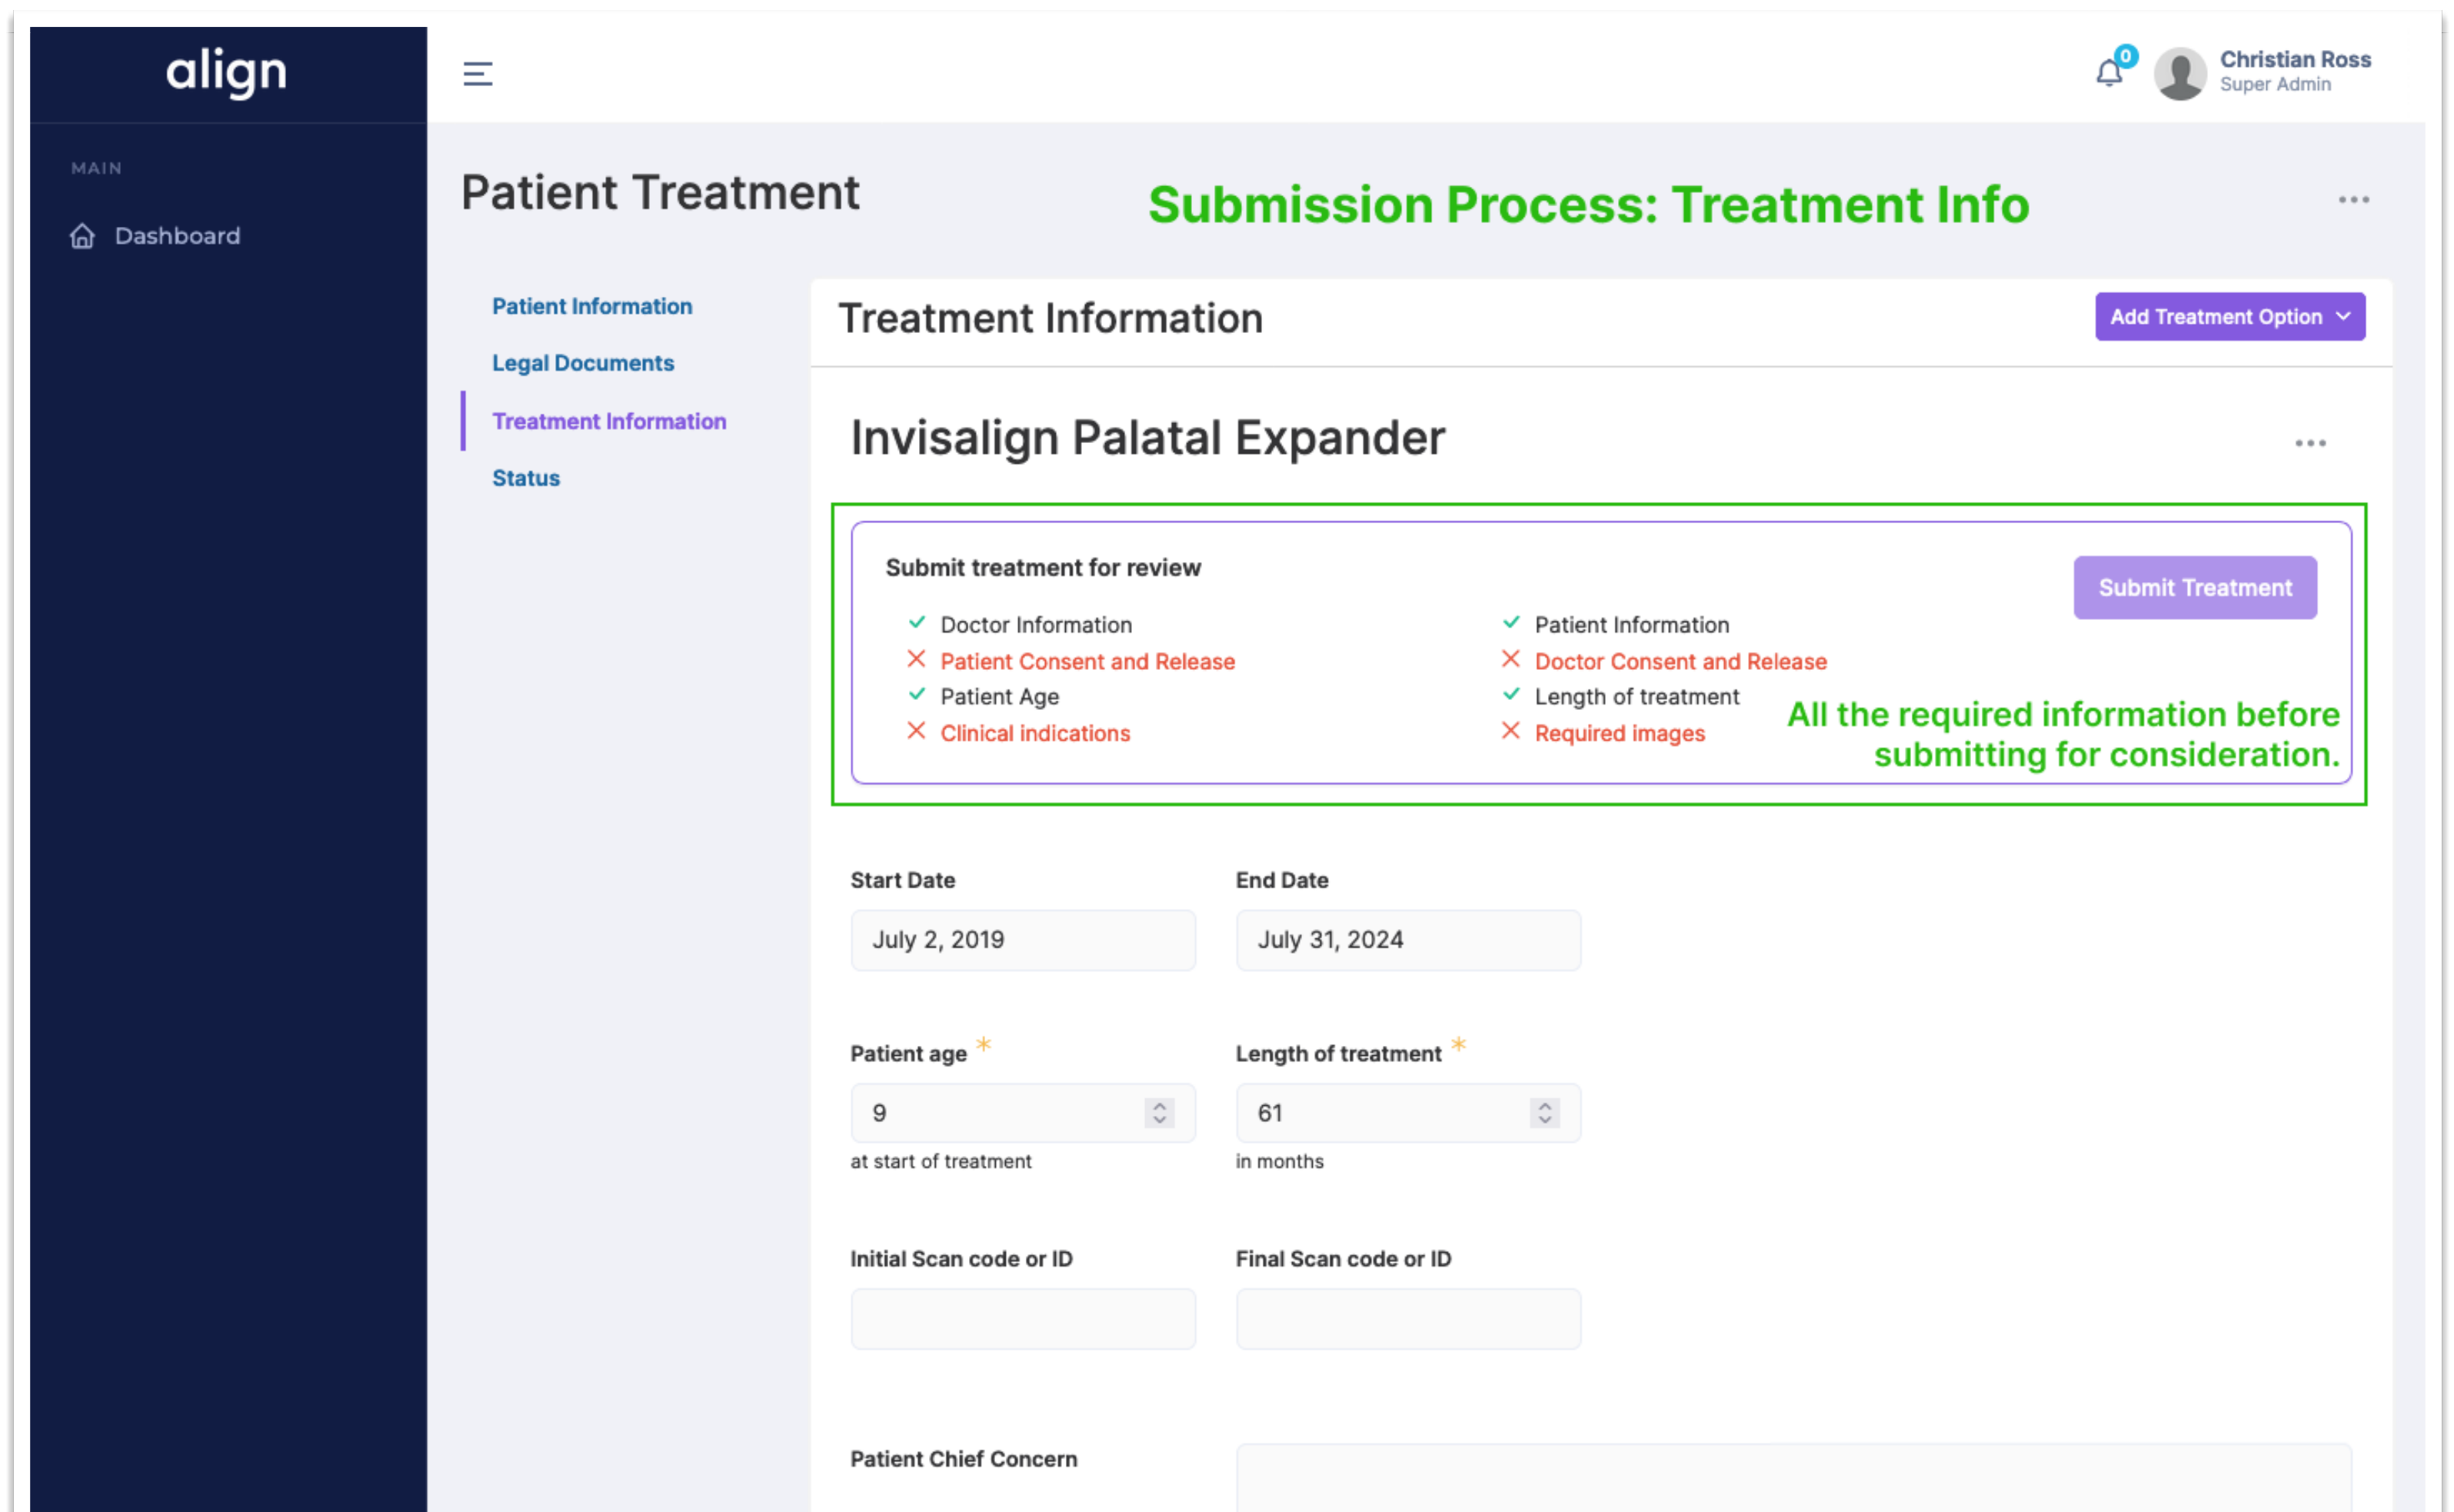

align

MAIN
Dashboard

Patient Treatment **Submission Process: Treatment Info**

Patient Information
Legal Documents
Treatment Information
Status

Treatment Information [Add Treatment Option](#)

Invisalign Palatal Expander

Submit treatment for review [Submit Treatment](#)

- ✓ Doctor Information
- ✗ Patient Consent and Release
- ✓ Patient Age
- ✗ Clinical Indications
- ✓ Patient Information
- ✗ Doctor Consent and Release
- ✓ Length of treatment
- ✗ Required images

All the required information before submitting for consideration.

Start Date: July 2, 2019 End Date: July 31, 2024

Patient age*: 9 at start of treatment Length of treatment*: 61 in months

Initial Scan code or ID: Final Scan code or ID:

Patient Chief Concern:

Submit for Review

Once you have uploaded and completed all of the fields for submission, your Submit Treatment button will be available to select.

Once a treatment has been submitted for review, no changes will be able to be made after that point. Please make sure all of your treatment and patient information is correct before submitting.

Click the Save button before proceeding.

The screenshot shows the 'align' software interface for submitting a treatment for review. The page title is 'Submission Process: Submit for Review'. The main content area is titled 'Treatment Information' and features a section for 'Invisalign Palatal Expander'. A checklist titled 'Submit treatment for review' shows that all required fields are completed, indicated by green checkmarks: Doctor Information, Patient Information, Patient Consent and Release, Doctor Consent and Release, Patient Age, Length of treatment, Clinical indications, and Required images. A purple 'Submit Treatment' button is highlighted with a green box and an arrow. Below the checklist, there are input fields for 'Start Date' (July 2, 2019) and 'End Date' (July 31, 2024). There are also dropdown menus for 'Patient age' (9) and 'Length of treatment' (61). At the bottom, there are fields for 'Initial Scan code or ID', 'Final Scan code or ID', and 'Patient Chief Concern'. A 'Save' button is located in the bottom right corner. The user's name, 'Christian Ross Super Admin', is visible in the top right corner.

Submit treatment for review

- ✓ Doctor Information
- ✓ Patient Information
- ✓ Patient Consent and Release
- ✓ Doctor Consent and Release
- ✓ Patient Age
- ✓ Length of treatment
- ✓ Clinical indications
- ✓ Required images

Submit Treatment

Start Date: July 2, 2019

End Date: July 31, 2024

Patient age: 9 at start of treatment

Length of treatment: 61 in months

Initial Scan code or ID

Final Scan code or ID

Patient Chief Concern


When required fields completed, you should be able to submit your treatment for review here

Published Treatments

You will be notified via email as your treatment is going through the review process. If a reviewer needs more information, they will request it and give you the ability to respond or complete.

Once the treatment is approved and published, it will then be live in the Align Global Gallery.

For questions or concerns, please email:
Barbara Grishaver
bgrishaver@aligntech.com

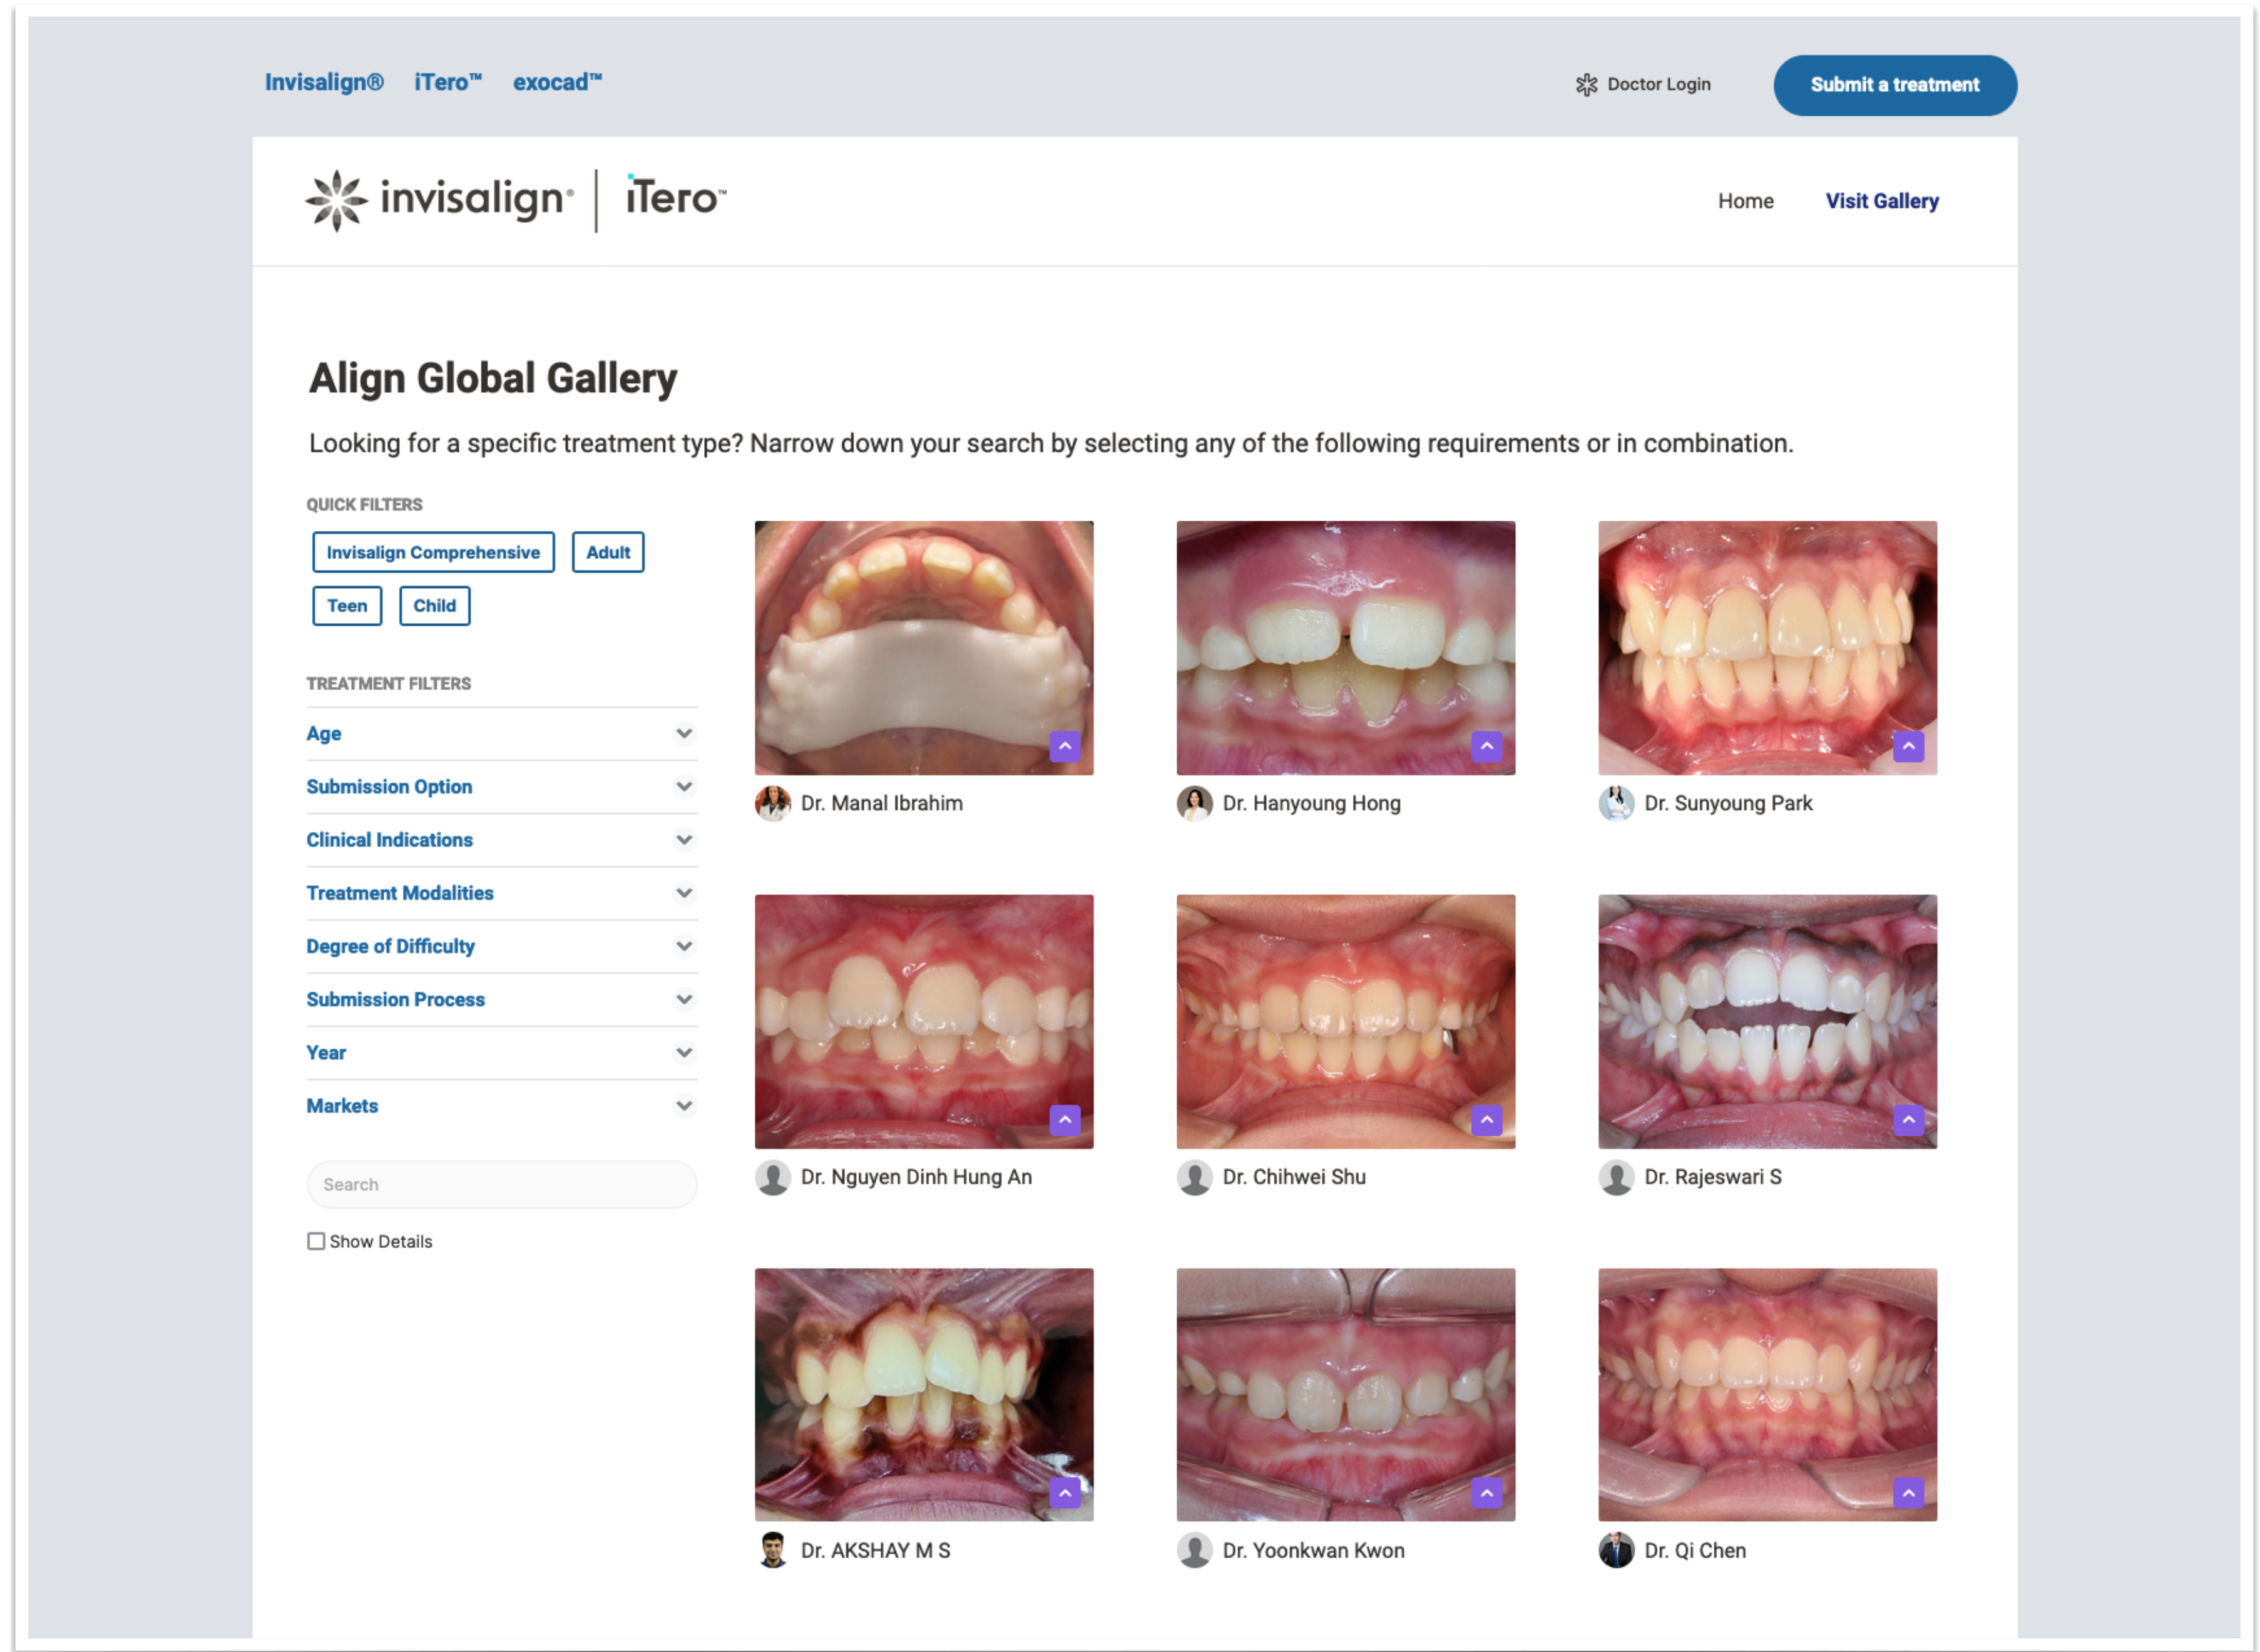

Invisalign® iTero™ exocad™

Doctor Login [Submit a treatment](#)

invisalign® | iTero™

Home [Visit Gallery](#)

Align Global Gallery

Looking for a specific treatment type? Narrow down your search by selecting any of the following requirements or in combination.

QUICK FILTERS

[Invisalign Comprehensive](#) [Adult](#)




[Teen](#) [Child](#)




TREATMENT FILTERS




[Age](#) [Submission Option](#) [Clinical Indications](#) [Treatment Modalities](#) [Degree of Difficulty](#) [Submission Process](#) [Year](#) [Markets](#)




Search




Show Details




  

 Dr. Manal Ibrahim  Dr. Hanyoung Hong  Dr. Sunyoung Park

 Dr. Nguyen Dinh Hung An  Dr. Chihwei Shu  Dr. Rajeswari S

 Dr. AKSHAY M S  Dr. Yoonkwan Kwon  Dr. Qi Chen